www.chromservis.eu/en/metamino-kit-manual




Safety Data Sheets (SDS) www.chromservis.eu/en/safety-data-sheets



# MetAmino<sup>®</sup> Sample Preparation Workflow


### Biological sample, (e.g. a biofluid serum, plasma)

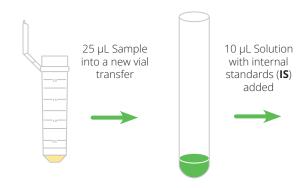


#### Note:

The sample preparation time can be reduced if all steps are performed in parallel. The detailed sample preparation procedure can be found in the User manual.

## Derivatization step

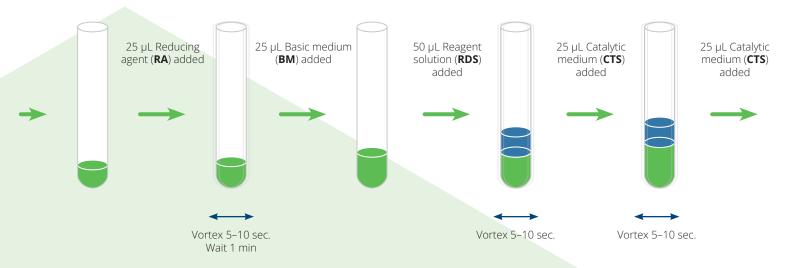

## Liquid-liquid extraction step

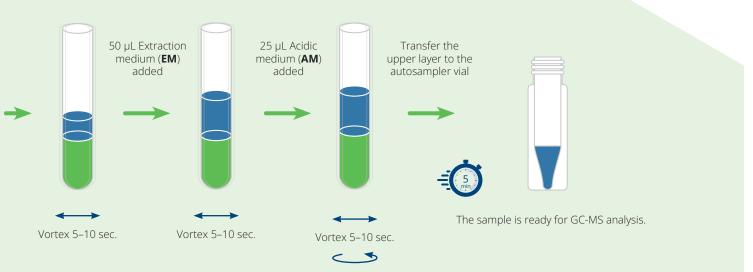

Centrifuge 30–60 sec. at 1500 × g